

Certificate of Analysis


EIA-4437	IL-1B-Elisa-CE	Lot Nr :	2205-5772
		Expiry Date :	12/02/2024

Tested composition :

Description	Lot nr.	Expiry Date
WASH-SOL	2201-4574/02	12/01/2027
ANTI-HRP	2202-4810/05	22/04/2024
ANTI	2202-4807/05	12/02/2024
CALIB 0	2105-2262/02	23/04/2026
DILUENT	2105-2259/04	23/04/2026
C1	2107-2930/05	11/07/2026
C2	2109-3350/01	21/08/2026
CALIB	2105-2263/03	24/04/2026
TMB-RTU	2105-2186/01	05/10/2024
STOP-SOL	2112-4186/01	02/12/2026

Results:

Parameter	Response mOD	B/T %	B/B0 %	Conc pg/ml	Range pg/ml
STD0 2105-2262/02	43.5				
STD1 2105-2263/03	137.0			15.8	
STD2 2105-2263/03	429.5			64.8	
STD3 2105-2263/03	1313.5			223.0	
STD4 2105-2263/03	2201.0			427.0	
STD5 2105-2263/03	2998.0			589.0	
C1 2107-2930 05	748.0			120.87	125.00 ± 30.00
C2 2109-3350 01	1754.5			317.42	330.00 ± 79.00

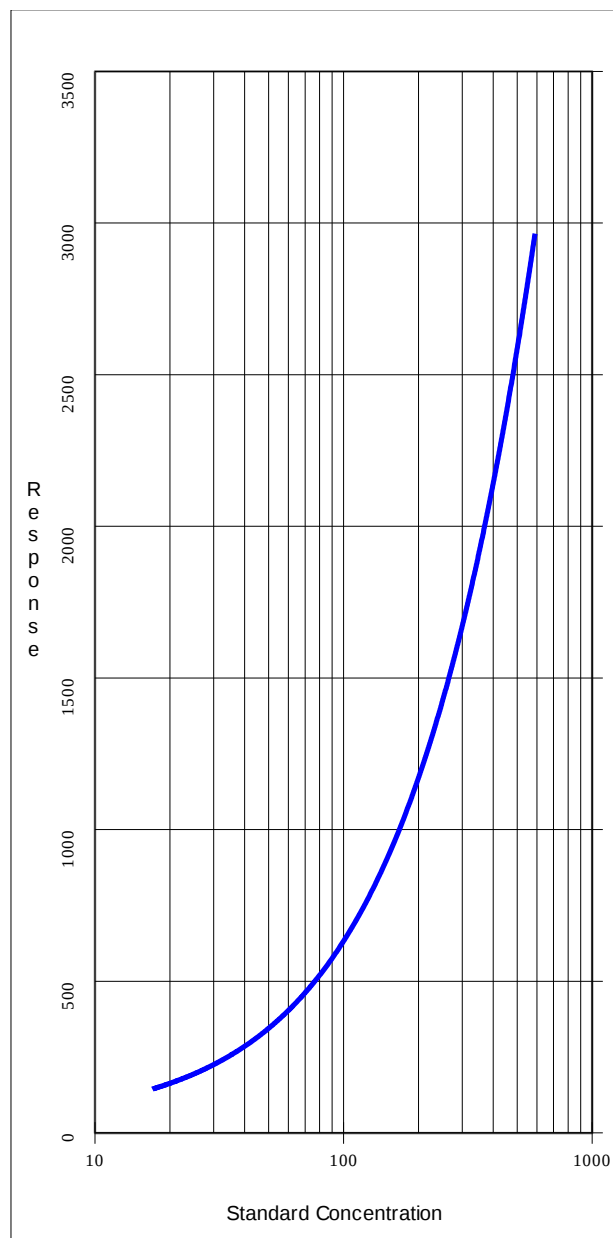

Only the figures before the slash should be taken into account for the batch identification.

ACCEPTED

Edition date : 31/05/2022

This document has been produced electronically and is valid without a signature.