


REV	ECO NUMBER	NAME
A	PR056827	M. GROBMAN

D

D

C

C

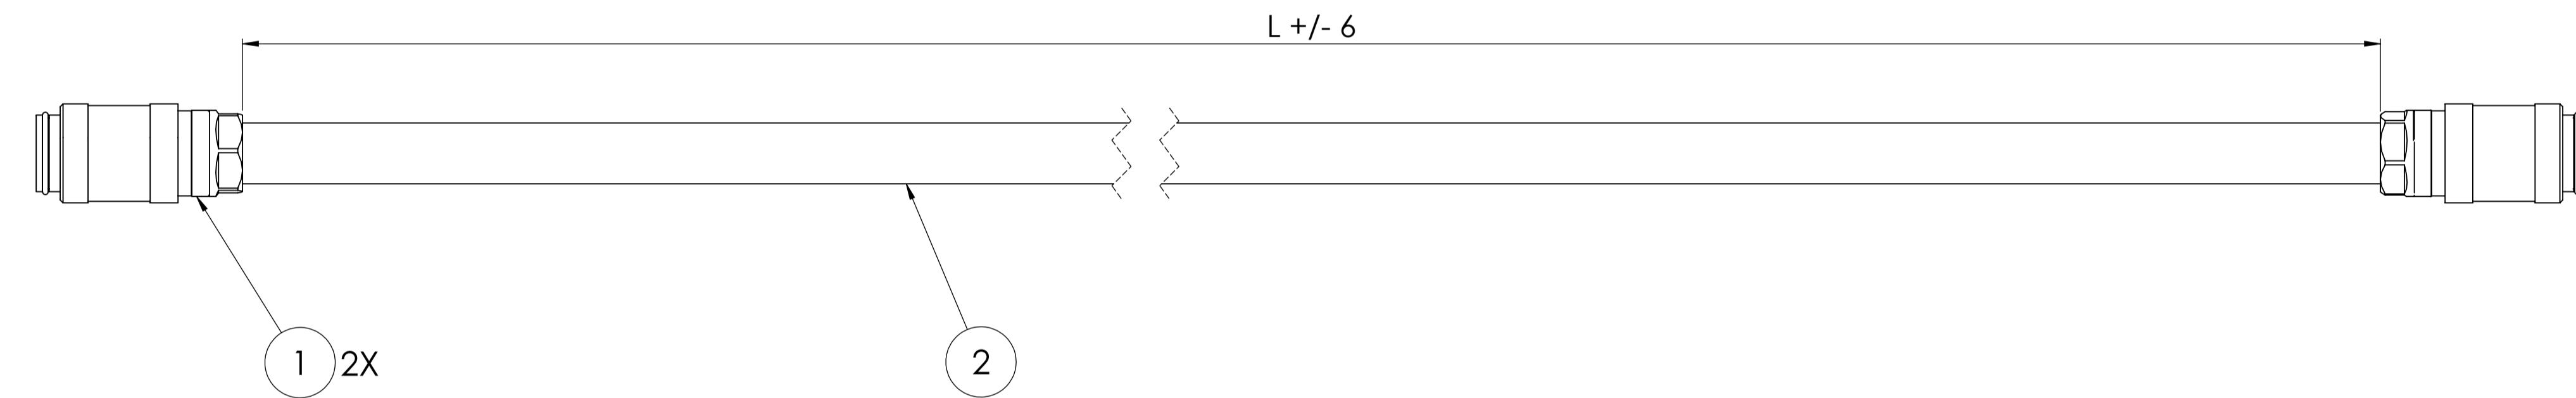

P/N	L (INCH)
712-0767-02	144
712-0900-02	108


ASSEMBLY INSTRUCTIONS:

1. INSERT BARBED END OF FITTINGS INTO THE HOSE. HOSE ENDS FIT FLUSH TO END OF FITTINGS.
2. THE AIR LEAKAGE SHALL NOT EXCEED A PRESSURE DROP OF 4 mmHg AT 300 mmHg FOR 1 MINUTE.
3. NEATLY COIL PRODUCT FOR PACKAGING.

THIS DOCUMENT CONTAINS PROPRIETARY TRADE SECRET AND CONFIDENTIAL INFORMATION WHICH IS THE PROPERTY OF SPACELABS HEALTHCARE. THIS DOCUMENT AND THE INFORMATION IT CONTAINS ARE NOT TO BE COPIED, DISTRIBUTED, OR DISCLOSED TO OTHERS, OR USED IN ANY MANNER OUTSIDE OF SPACELABS HEALTHCARE WITHOUT PRIOR WRITTEN APPROVAL OF SPACELABS HEALTHCARE.

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES, TOLERANCES AS SHOWN BELOW

LINEAR	ANGULAR
X.X ± 0.25	± 1 °
X.XX ± 0.25	
X.XXX ± 0.25	
X.XXXX ± 0.0625	



GENERAL THREAD FIT 6H 6g

Spacelabs Healthcare

DESCRIPTION

DRAWING FOR ADULT NIBP HOSE

SIZE

PART NUMBER

REV

A1 653-1659-00 A

VERSION:

SHEET 1 OF 1